

(12) INTERNATIONAL APPLICATION PUBLISHED UNDER THE PATENT COOPERATION TREATY (PCT)

(19) World Intellectual Property
Organization
International Bureau



(43) International Publication Date
21 October 2004 (21.10.2004)

PCT

(10) International Publication Number
WO 2004/090564 A1

(51) International Patent Classification⁷: **G01R 33/563**

(21) International Application Number:
PCT/IB2004/050397

(22) International Filing Date: 5 April 2004 (05.04.2004)

(25) Filing Language: English

(26) Publication Language: English

(30) Priority Data:
03100995.4 14 April 2003 (14.04.2003) EP

(71) Applicant (for all designated States except US): **KONINKLIJKE PHILIPS ELECTRONICS N.V.** [NL/NL];
Groenewoudseweg 1, NL-5621 BA Eindhoven (NL).

(72) Inventors; and

(75) Inventors/Applicants (for US only): **VAN MUISWINKEL, Arianne, M., C.** [NL/NL]; c/o Prof. Holstlaan 6, NL-5656 AA Eindhoven (NL).
HOLTHUIZEN, Ronaldus, F., J. [NL/NL]; c/o Prof. Holstlaan 6, NL-5656 AA Eindhoven (NL).
HOOGENRAAD, Frank, G., C. [NL/NL]; c/o Prof. Holstlaan 6, NL-5656 AA Eindhoven (NL).

(74) Agent: **COHEN, Julius, S., Prof.** Holstlaan 6, NL-5656 AA Eindhoven (NL).

(81) Designated States (unless otherwise indicated, for every kind of national protection available): AE, AG, AL, AM,

AT, AU, AZ, BA, BB, BG, BR, BW, BY, BZ, CA, CH, CN, CO, CR, CU, CZ, DE, DK, DM, DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, HR, HU, ID, IL, IN, IS, JP, KE, KG, KP, KR, KZ, LC, LK, LR, LS, LT, LU, LV, MA, MD, MG, MK, MN, MW, MX, MZ, NA, NI, NO, NZ, OM, PG, PH, PL, PT, RO, RU, SC, SD, SE, SG, SK, SL, SY, TJ, TM, TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, YU, ZA, ZM, ZW.


(84) Designated States (unless otherwise indicated, for every kind of regional protection available): ARIPO (BW, GH, GM, KE, LS, MW, MZ, SD, SL, SZ, TZ, UG, ZM, ZW), Eurasian (AM, AZ, BY, KG, KZ, MD, RU, TJ, TM), European (AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR, GB, GR, HU, IE, IT, LU, MC, NL, PL, PT, RO, SE, SI, SK, TR), OAPI (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW, ML, MR, NE, SN, TD, TG).

Declaration under Rule 4.17:

— as to applicant's entitlement to apply for and be granted a patent (Rule 4.17(ii)) for the following designations AE, AG, AL, AM, AT, AU, AZ, BA, BB, BG, BR, BW, BY, BZ, CA, CH, CN, CO, CR, CU, CZ, DE, DK, DM, DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, HR, HU, ID, IL, IN, IS, JP, KE, KG, KP, KR, KZ, LC, LK, LR, LS, LT, LU, LV, MA, MD, MG, MK, MN, MW, MX, MZ, NA, NI, NO, NZ, OM, PG, PH, PL, PT, RO, RU, SC, SD, SE, SG, SK, SL, SY, TJ, TM, TN, TR, TT, TZ, UA, UG, UZ, VC, VN, YU, ZA, ZM,

[Continued on next page]

(54) Title: **SYSTEM AND METHOD FOR DETECTING FIBRE TRACTS**

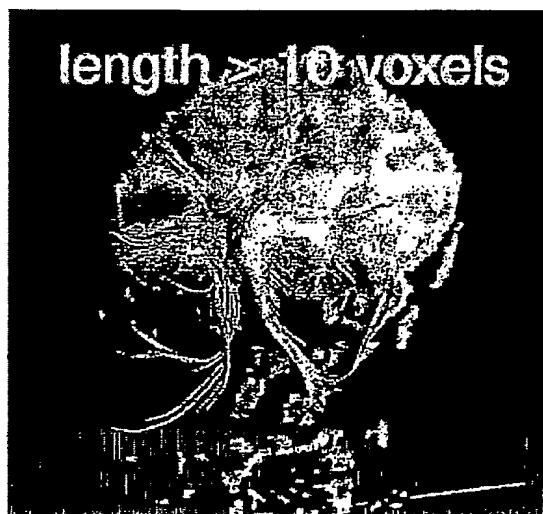

(57) Abstract: The invention relates to a system for displaying fibre tracts of a human or animal, comprising memory means holding diffusion images of a region of interest of said human or animal, processing means connected to the memory means for deriving fibre tract data from the diffusion images, and display means for displaying the fibre tracts derived by the processing means wherein the processing means include a discriminator to select the fibre tract data to be displayed on the display means.

WO 2004/090564 A1



ZW, ARIPO patent (BW, GH, GM, KE, LS, MW, MZ, SD, SL, SZ, TZ, UG, ZM, ZW), Eurasian patent (AM, AZ, BY, KG, KZ, MD, RU, TJ, TM), European patent (AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR, GB, GR, HU, IE, IT, LU, MC, NL, PL, PT, RO, SE, SI, SK, TR), OAPI patent (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW, ML, MR, NE, SN, TD, TG)

Published:

— with international search report

For two-letter codes and other abbreviations, refer to the "Guidance Notes on Codes and Abbreviations" appearing at the beginning of each regular issue of the PCT Gazette.

System and method for detecting fibre tracts

The invention relates to a system for detecting fibre tracts of a human or animal, comprising memory means for holding diffusion images of a region of interest of said human or animal, first processing means connected to the memory means for deriving fibre tract data from the diffusion images, and second processing means for processing the
5 fibre tracts derived by the first processing means.

Such a system is known from JP-A-11-000320.

In this known system the first processing means deduce a highest direction of a diffusion coefficient with a pre-determined point as a starting point using a diffusion tensor at each point of the image and deducing the next point located at a position that is a pre-
10 determined distance apart in that direction, and continuing this process with a deduced next point as the starting point for the next step. The display means of this system serve as the second processing means of the fibre tracks and merely display all points derived by this known method, resulting in an image which is considered to represent the nerve fibres that are actually present.

15 A problem with this known system is that the displayed information is not entirely accurate due to noise or other causes which results in the display of fibres that are spurious or otherwise of no interest.

In this connection it is remarked that the diffusion images are the result of indirect measurements such as obtained by magnetic resonance imaging.

20 Magnetic resonance imaging is known in the art in general. The application of magnetic resonance imaging for fibre tracking is known from WO-A-01/91639.

From this publication WO-A-01/91639 it is known to initiate fibre tracking by selecting a pixel from a diffusion tensor magnetic resonance image, to connect the pixels and to effect a judgement regarding termination of the pixel tracking, which in each direction is
25 based upon the randomness of the fibre orientation of the adjacent pixels. The technology disclosed in this document suffers however from the same problem as JP-A-11-000320, i.e. the processing or display of spurious fibres.

The invention is aimed to resolve this problem.

According to the invention the system for detecting fibre tracts of a human or animal is characterized in that the first processing means includes a discriminator to select the fibre tract data to be processed by the second processing means. The second processing means can be used for several purposes, for instance to execute statistical analysis on the data, or to effect that the fibre tract data are displayed on display means.

By the application of the discriminator the validity of the fibre tract data can be vastly improved.

This can particularly be accomplished in a system which according to a preferred embodiment is characterized in that the discriminator prevents selecting fibre tract data that jointly represent a fibre tract or fibre tracts of less than a pre-determined length. The discriminator regards fibre tracts of less than the pre-determined length as being invalid. Such too short fibre tracts are considered to be spurious which consequently need not be available for further processing such as displaying.

In a further aspect of the invention the system is characterized in that the discriminator prevents selecting fibre tract data that jointly represent a bundle of fibre tracts of less than a pre-determined number of fibre tracts per surface area or per volume. This measure rules out the display of single erroneous tracts.

The invention is also embodied in a method of detecting fibre tracts of a human or animal in which diffusion image data of a region of interest of such human or animal are processed to derive fibre tract data that are thereafter further processed, for instance displayed.

The method of the invention is characterized in that further processing of the fibre tract data is restricted to such fibre tract data that jointly represent a fibre tract or fibre tracts that satisfy at least one pre-determined criterion.

In a first preferred embodiment of the invention the method is characterized in that a first pre-determined criterion is selected to represent a minimum-length of the fibre tract or fibre tracts.

In a second preferred embodiment which may be combined with the first preferred embodiment, the method is characterized in that a second pre-determined criterion is selected to represent a minimum number of fibre tracts per surface area or volume that are part of a bundle of fibre tracts.

When indeed the first pre-determined criterion and the second pre-determined criterion are employed in combination, the method may automatically yield all fibre bundles in the tissue being examined. This tissue under examination may furthermore be compared to

a standard data set in order to improve the reliability of the fibre tracking according to the invention.

Results of the invention are shown hereafter with reference to an exemplary embodiment of a system according to the invention, in which diffusion tensor magnetic
5 resonance images are processed in order to obtain fibre tracts. The invention further relates to a computer programme as defined in Claim 7. The computer programme of the invention may be downloaded into a system for detecting fibre tracks so as to enable the system to carry out the method of the invention. The computer programme may be supplied on a data carrier such as a CD-rom, or may be downloaded from a data network, such as the world-
10 wide web.

Figure 1 shows the system according to the invention.

Figures 2 to 5 show some results obtained with the system according to the
15 invention.

With reference to figure 1 the system according to the invention is indicated with reference number 1. This system for detecting fibre tracts of a human or animal
20 comprises memory means (2) for holding diffusion images of a region of interest of said human or animal. The images can be derived for instance with magnetic resonance imaging which is known to the person skilled in the art and which requires therefore no further elucidation.

The memory means (2) are connected to first processing means (3) which
25 operates on the diffusion images that are held in the memory means (2). The first processing means (3) are connected to second processing means, in this example display means (4) for displaying the fibre tracts that are derived from the diffusion images by the first processing means (3). To this end the first processing means (3) includes a discriminator to select the fibre tract data that are to be displayed on the display means (4). The results are
30 comparatively shown in the following figures.

Figure 2 shows the image visualised on the display when the discriminator is not employed.

Figures 3, 4 and 5 show the image being visualised on the display means when the discriminator is active to display only fibre tract data that represent a minimum-length of the fibre tract or fibre tracts to be displayed.

In figure 3 the minimum-length of the fibre tracts to be displayed amounts to
5 10 voxels.

In figure 4 the said minimum-length amounts to 20 voxels whereas in figure 5 the said minimum-length amounts to 30 voxels.

As a result of the invention the display of undesired short fibres is prevented and the recognition of bundles of fibres can take place more easy.

CLAIMS:

1. System for detecting fibre tracts of a human or animal, comprising memory means for holding diffusion images of a region of interest of said human or animal, first processing means connected to the memory means for deriving fibre tract data from the diffusion images, and second processing means for processing the fibre tracts derived by the first processing means, characterized in that, the first processing means includes a discriminator to select the fibre tract data to be processed by the second processing means.
2. System according to claim 1, characterized in that, the discriminator prevents selecting fibre tract data that jointly represent a fibre tract or fibre tracts of less than a pre-determined length.
3. System according to claim 1 or 2, characterized in that, the discriminator prevents selecting fibre tract data that jointly represent a bundle of fibre tracts of less than a pre-determined number of fibre tracts per surface area or per volume.
4. Method of detecting fibre tracts of a human or animal comprising the steps of
 - processing diffusion image data of a region of interest of said human or animal to derive fibre tract data;
 - processing the fibre tract datacharacterized in that, processing the fibre tract data is restricted to such fibre tract data that jointly represent a fibre tract or fibre tracts that satisfy at least one pre-determined criterion.
5. Method according to claim 4, characterized in that, a first pre-determined criterion is selected to represent a minimum-length of the fibre tract or fibre tracts.
6. Method according to claim 4 or 5, characterized in that, a second pre-determined criterion is selected to represent a minimum number of fibre tracts per surface area or volume that are part of a bundle of fibre tracts to be processed.

7. Computer programme for detecting fibre tracts of a human or animal
5 comprising instructions for
- processing diffusion image data of a region of interest of said human or animal to derive fibre tract data;
 - processing the fibre tract data
- characterized in that, processing the fibre tract data is restricted to such fibre tract data that
10 jointly represent a fibre tract or fibre tracts that satisfy at least one pre-determined criterion.

1/3

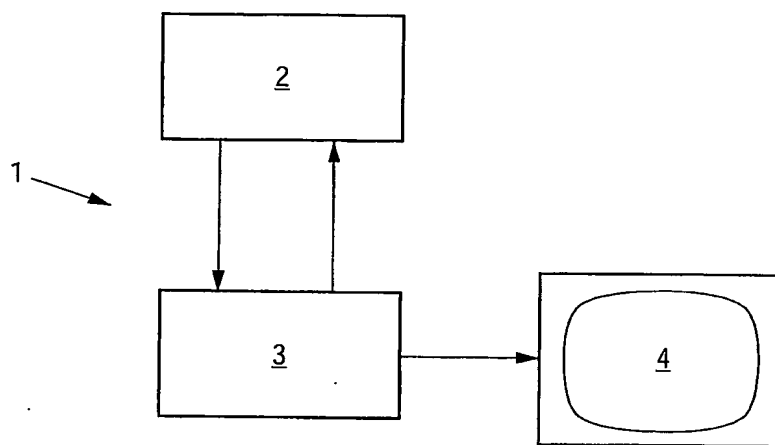


FIG.1

2/3

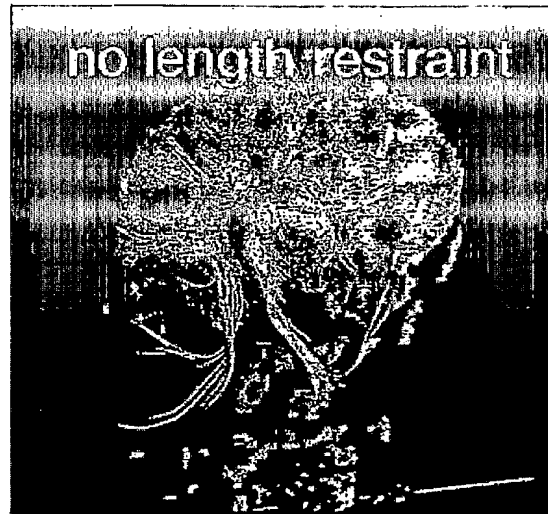


FIG. 2

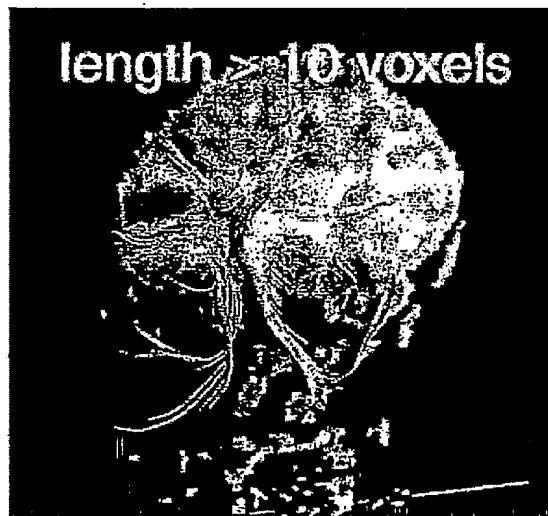


FIG. 3

3/3

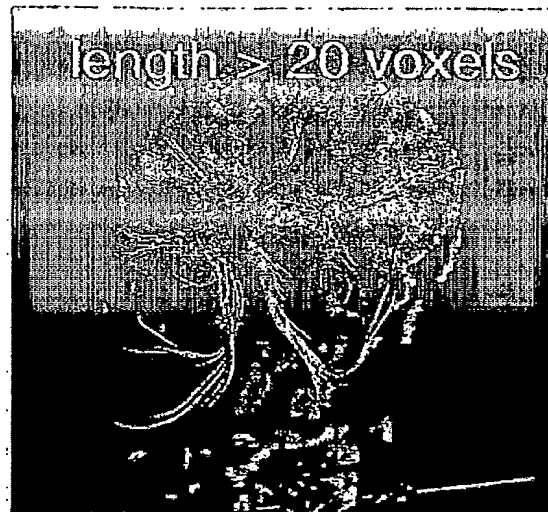


FIG.4

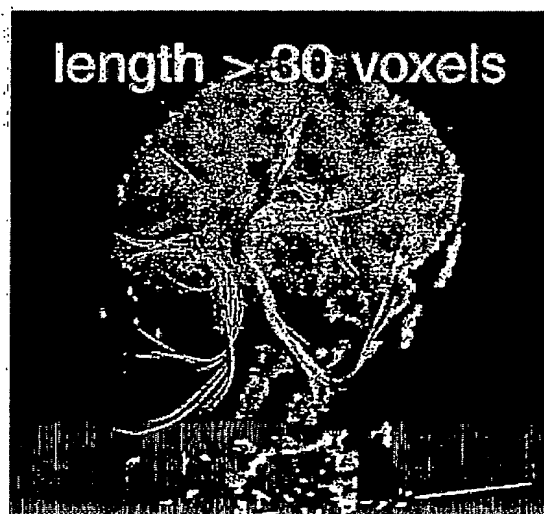


FIG.5

INTERNATIONAL SEARCH REPORT

International Application No

IB/IB2004/050397

C.(Continuation) DOCUMENTS CONSIDERED TO BE RELEVANT

Category *	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
X	KIM K.H. ET AL: "A Novel Fiber-Tracking Method Using Vector Criterion and Predictive Directivity in Diffusion Tensor Imaging" PROCEEDINGS OF THE ISMRM, TENTH MEETING PROCEEDINGS, 18 May 2002 (2002-05-18), XP002289090 HONOLULU, HI, USA the whole document	4
X	STIELTJES B ET AL: "Diffusion tensor imaging and axonal tracking in the human brainstem." NEUROIMAGE. SEP 2001, vol. 14, no. 3, September 2001 (2001-09), pages 723-735, XP002289186 ISSN: 1053-8119 page 725 - page 727	1,4,7
A	MORI SUSUMU ET AL: "Fiber tracking: principles and strategies - a technical review." NMR IN BIOMEDICINE. 2002 NOV-DEC, vol. 15, no. 7-8, November 2002 (2002-11), pages 468-480, XP009034056 ISSN: 0952-3480 * section "Erroneous results due to noise and resolution limitations" *	1-7

THIS PAGE BLANK (USPTO)